



# Technical differences between USP and USP Twist

## ULTRA SAFETY PLUS

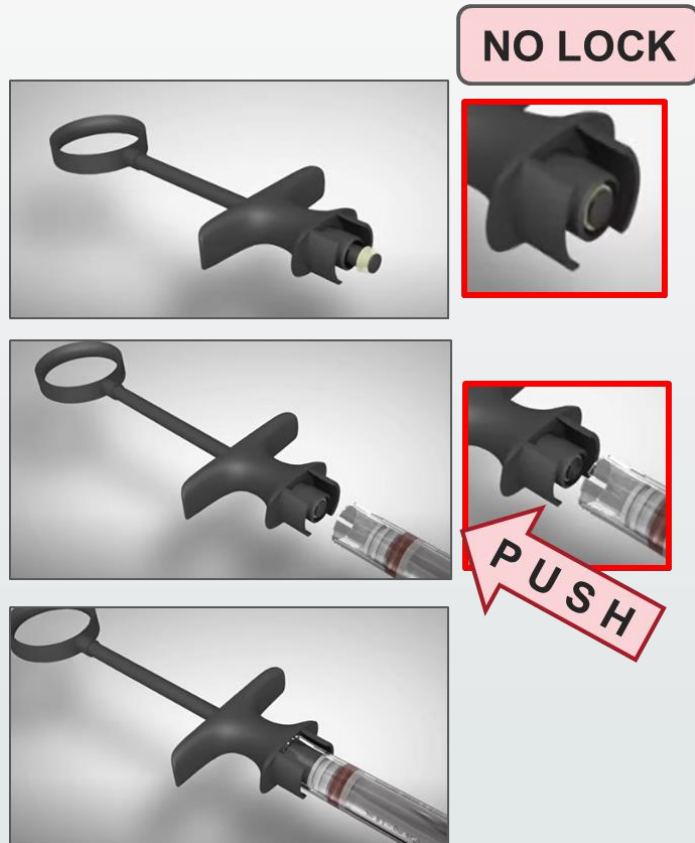

## ULTRA SAFETY PLUS TWIST

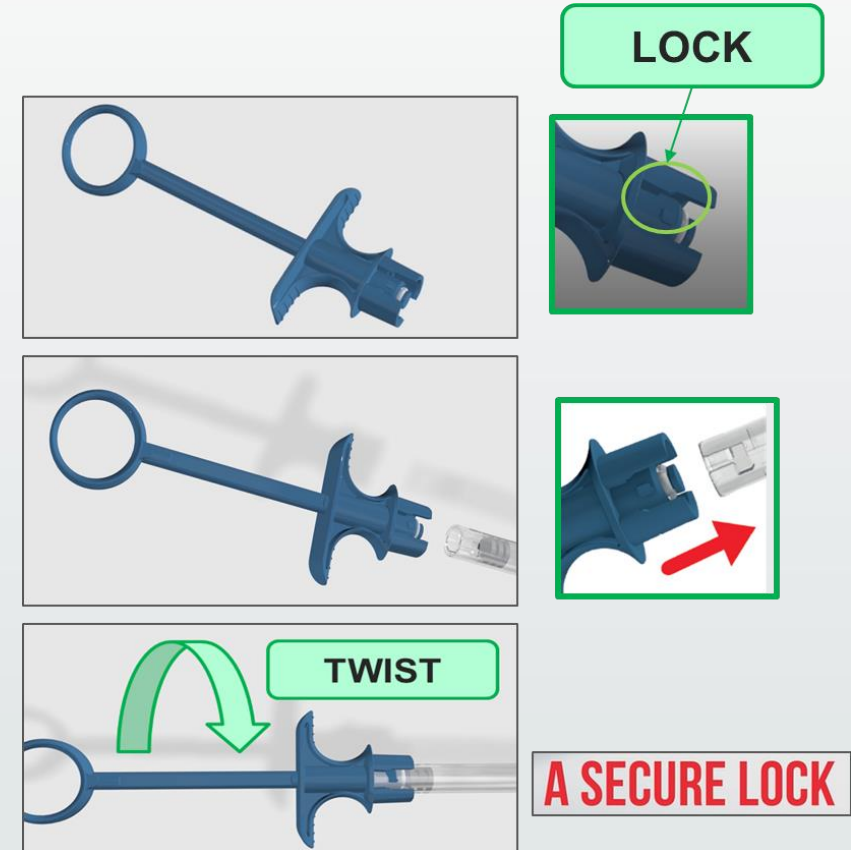

« Be cautious to keep the device assembled whenever you move the protective sheath and during the injection »